

zumax

Zumax Medical
Beyond Vision




**Removal kit for
instrument separation**

Instrument separation is one of the most common complications in root canal treatment process. The innovative design of instrument separation removal kit changes the traditional clinical methods. This design makes instrument separation removal process quick and easy.


Advantages:

- Limited amount of removed dentin of root canal wall
- Avoid the inconvenience and risk of the ultrasonic tip fracture in traditional technique
- Avoid secondary fracture of the separated nickel titanium instrument when using the ultrasonic technique
- Microscopic tweezers are favorable and efficient for operation
- The operation process is easy to learn and use

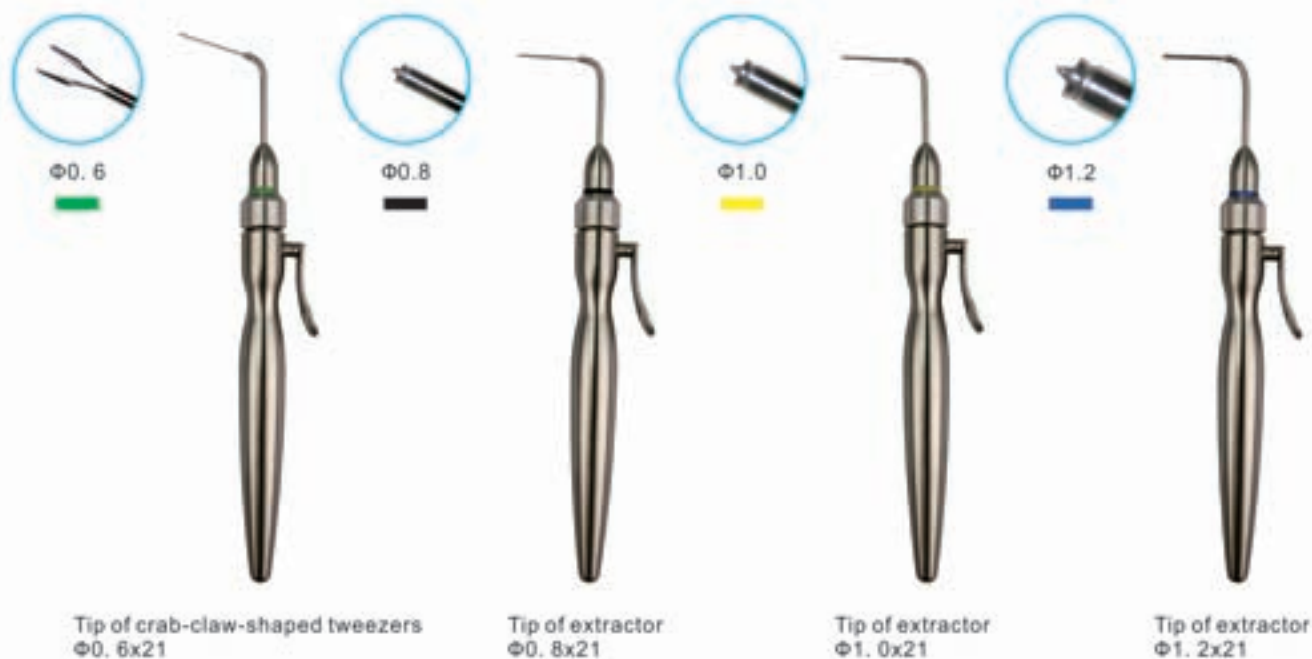



Trephine bur, L:17mm

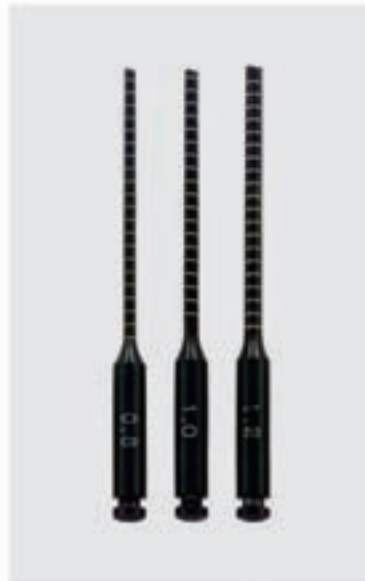

Trephine bur, L:21mm



Trephine bur, L:25mm

Item No.	Description	Item No.	Description
FT0017	Instrument separation removal kit, 17mm	NX0617	Tip of crab-claw-shaped tweezers $\Phi 0.6 \times 17$
FT0021	Instrument separation removal kit, 21mm	NX0621	Tip of crab-claw-shaped tweezers $\Phi 0.6 \times 21$
FT0025	Instrument separation removal kit, 25mm	NX0625	Tip of crab-claw-shaped tweezers $\Phi 0.6 \times 25$
NB0001	Handle of extractors and tweezers	C0817	Trephine bur $\Phi 0.8 \times 17$
NT0817	Tip of extractor $\Phi 0.8 \times 17$	C1017	Trephine bur $\Phi 1.0 \times 17$
NT1017	Tip of extractor $\Phi 1.0 \times 17$	C1217	Trephine bur $\Phi 1.2 \times 17$
NT1217	Tip of extractor $\Phi 1.2 \times 17$	C0821	Trephine bur $\Phi 0.8 \times 21$
NT0821	Tip of extractor $\Phi 0.8 \times 21$	C1021	Trephine bur $\Phi 1.0 \times 21$
NT1021	Tip of extractor $\Phi 1.0 \times 21$	C1221	Trephine bur $\Phi 1.2 \times 21$
NT1221	Tip of extractor $\Phi 1.2 \times 21$	C0825	Trephine bur $\Phi 0.8 \times 25$
NT0825	Tip of extractor $\Phi 0.8 \times 25$	C1025	Trephine bur $\Phi 1.0 \times 25$
NT1025	Tip of extractor $\Phi 1.0 \times 25$	C1225	Trephine bur $\Phi 1.2 \times 25$
NT1225	Tip of extractor $\Phi 1.2 \times 25$		



ZUMAX MEDICAL CO., LTD.

5 Zhiying Street, Suzhou New District
Jiangsu, China 215129
Tel: +86 512 66650512 ext. 502/504/510
Fax: +86 512 666909655
Email: sales@zumaxmedical.com
Http: [//www.zumaxmedical.com](http://www.zumaxmedical.com)

